

Specifications (measured @ Ta= 25°C, 250VAC, full load and after warm-up)

REGULATIONS		
Parameter	Condition	Value
Output Accuracy	230VAC, full load	±1.0%
Line Regulation	low line to high line, full load	±0.2%
Load Regulation	0% to 100% load	0.5% max.
	10% to 100% load	0.4% max.
Transient Peak Deviation	load step from 50% - 75% change at 2.5A/μs	3.0% Vout max.
Transient Recovery Time	load step from 50% - 75% change at 2.5A/μs	500μs typ.

PROTECTIONS			
Parameter	Condition	Value	
Input Fuse	internal line and neutral	T3.15A / 250VAC, slow blow type	
Short Circuit Protection (SCP)		continuous, auto-recovery	
Over Load Protection (OLP)	% of Iout rated (Hiccup)	115% min. / 150% max.	
Over Voltage Protection (OVP)	% of Vout nominal (Latch off)	115% min. / 135% max.	
Isolation Voltage ⁽⁶⁾	tested for 1 minute	I/P to O/P	4kVAC
		I/P to Case	1.5kVAC
		O/P to Case	1.5kVAC
Isolation Resistance	500VDC	100MΩ min.	
Insulation Grade		reinforced	
Leakage Current	264VAC	75μA max.	
Means of Protection	working voltage 250VAC/continuous	2MOPP	
Medical Device Classification		built-in power supply	
Internal	clearance	>8.0mm	
	creepage	>8.0mm	

Notes:
 Note5: For repeat Hi-Pot testing, reduce the time and/or the test voltage



ENVIRONMENTAL			
Parameter	Condition	Value	
Operating Temperature Range	refer to derating graph	-25°C to +85°C	
	full load, 230VAC	enclosed	-25°C to +60°C
		open frame	-25°C to +55°C
Temperature Coefficient		±0.02%/K	
Operating Altitude		5000m max.	
Operating Humidity	non-condensing	5% to 95% RH	
Pollution Degree		PD2	
Thermal Shock		MIL-STD-810F	
Shock		IEC60068-2-27	
Vibration		IEC60068-2-6	
MTBF	according to MIL-HDBK-217F, full load, +25°C	790.3 x 10 ³ hours	

continued on next page

Specifications (measured @ Ta= 25°C, 250VAC, full load and after warm-up)

Derating Graph

(@ Chamber and natural convection 0.1m/s)

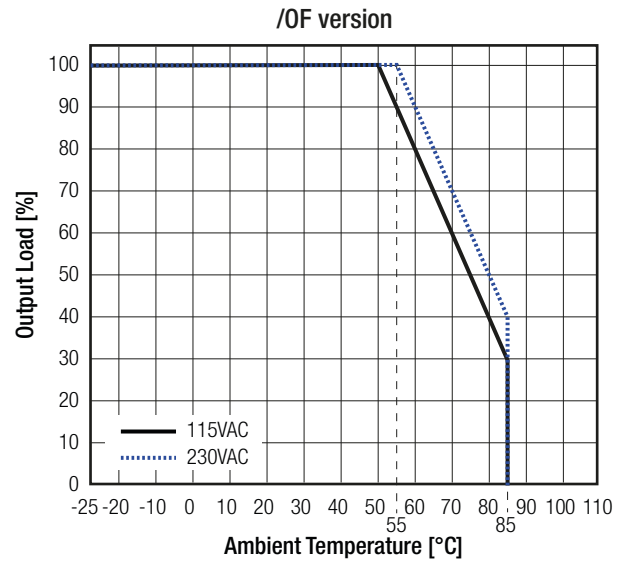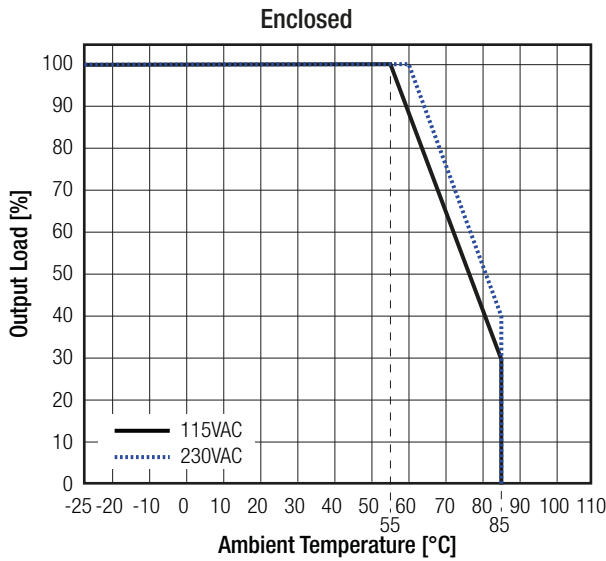

SAFETY AND CERTIFICATIONS

Certificate Type (Safety)	Report / File Number	Standard
Medical Electric Equipment, General Requirements for Safety and Essential Performance	E314885	CAN/CSA-C22.2 No. 60601-1:14 ANSI/AAMI ES60601-1:2005 + A2:2010
Medical Electric Equipment, General Requirements for Safety and Essential Performance (CB Scheme)	1408016004	IEC60601-1:2005 + C2:2007, 3rd Edition EN60601-1:2006
Information Technology Equipment - General Requirements for Safety (LVD)	TW1708008-001	EN60950-1:2006 + A2:2013
Information Technology Equipment - General Requirements for Safety		IEC60950-1:2005, 2nd Edition + A2:2013
EAC	RU-AT.49.09571	TP TC 004/2011 TP TC 004/2011
RoHs2+		RoHS-2011/65/EU + AM-2015/863

EMC Compliance (Medical)	Conditions	Standard / Criterion
Medical electrical equipment - Part 1-2: General requirements for basic safety and essential performance - Collateral standard: Electromagnetic compatibility - Requirements and tests		EN60601-1-2:2015
Industrial, scientific and medical equipment – Radio frequency disturbance characteristics – Limits and methods of measurement		EN55011:2009 + A1:2010 Class B Conducted, Class A Radiated
Industrial, scientific and medical equipment - Radio frequency disturbance characteristics - Limits and methods of measurement		CISPR11:2009 + A1:2010 Class B Conducted, Class A Radiated
ESD Electrostatic discharge immunity test	Air ±15kV; Contact ±8kV	IEC61000-4-2:2008
Radiated, radio-frequency, electromagnetic field immunity test	10V/m (80-2700MHz) 27V/m (385MHz) 28V/m (450MHz)	IEC61000-4-3:2006 + A2:2010
Fast Transient and Burst Immunity	AC Power Port: ±2kV	IEC61000-4-4:2012
Surge Immunity	AC Port: L-N= ±1kV L-GND= ±2kV	IEC61000-4-5:2005
Immunity to conducted disturbances, induced by radio-frequency fields	6Vr.m.s	IEC61000-4-6:2013
Power Frequency Magnetic Field	50Hz, 30A/m	IEC61000-4-8:2009
Voltage Dips and Interruptions	Dips: >95%; 30%; Interruptions >95%	IEC61000-4-11:2004
Limits of Harmonic Current Emissions		EN61000-3-2:2005 + A2:2009, Class D
Limits of Voltage Fluctuations and Flicker		EN61000-3-3:2013

continued on next page