

## 2 Specifications Charts

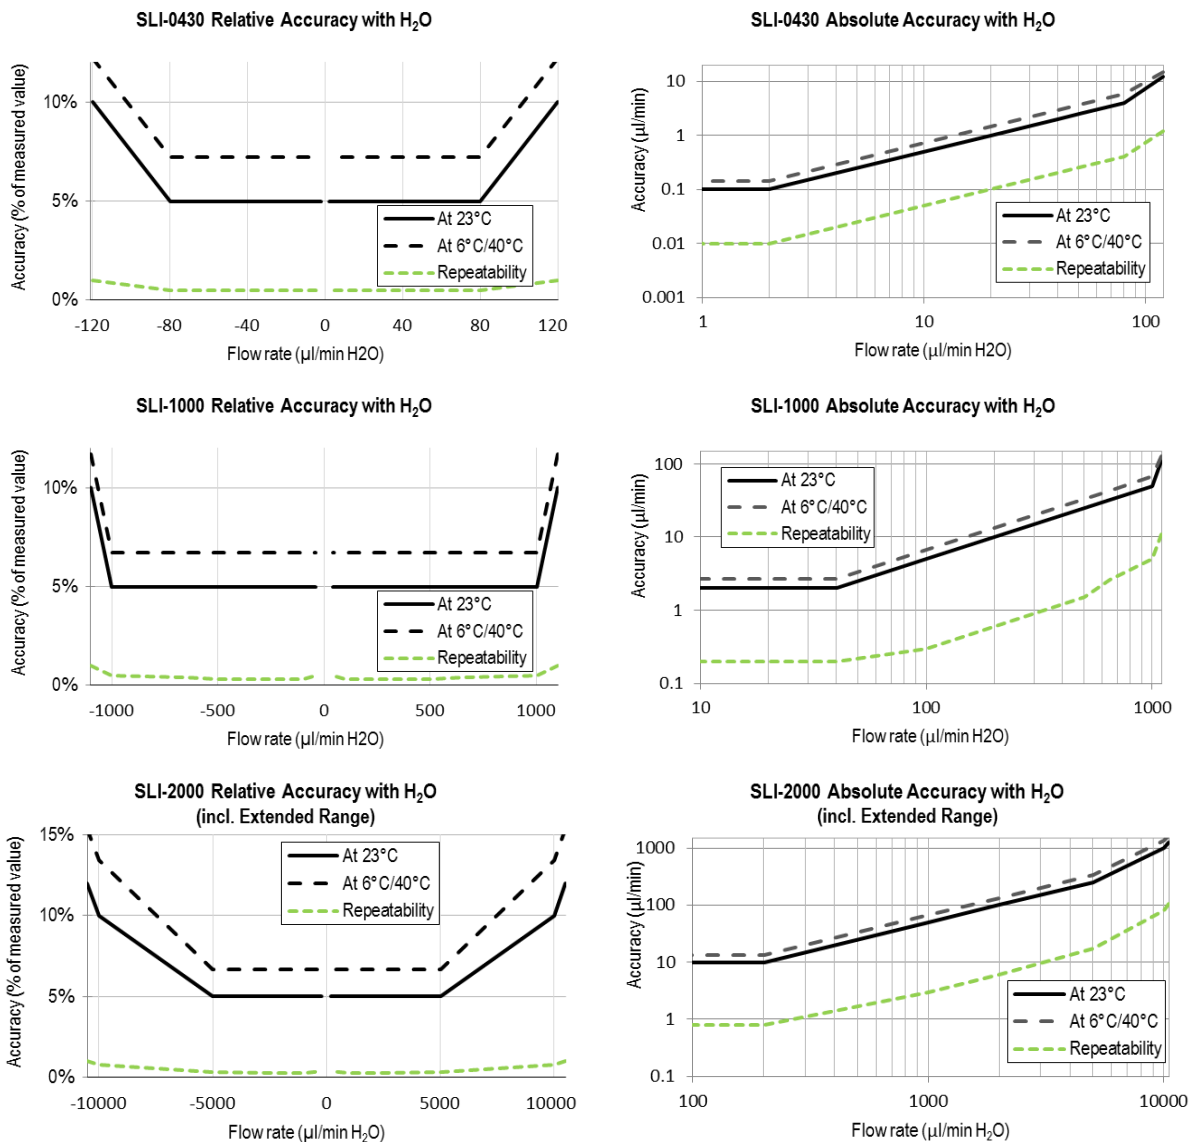


Figure 1: Flow meter accuracy and repeatability across the flow range. Relative error in % of measured value (left column) and absolute error in µl/min (right column) for H<sub>2</sub>O

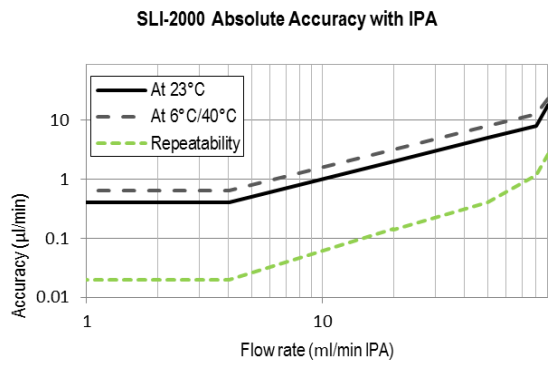
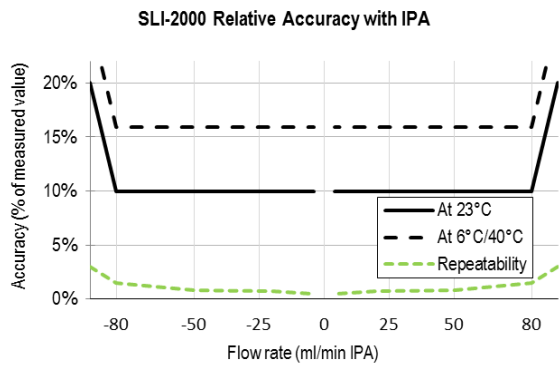
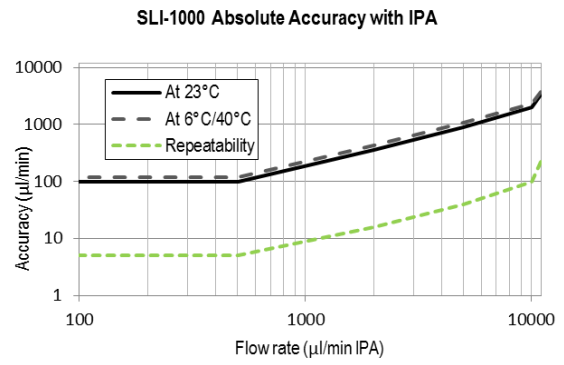
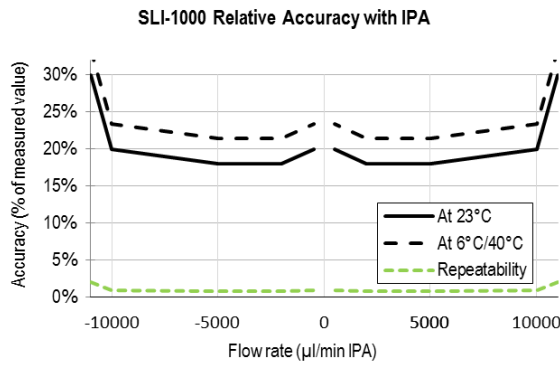
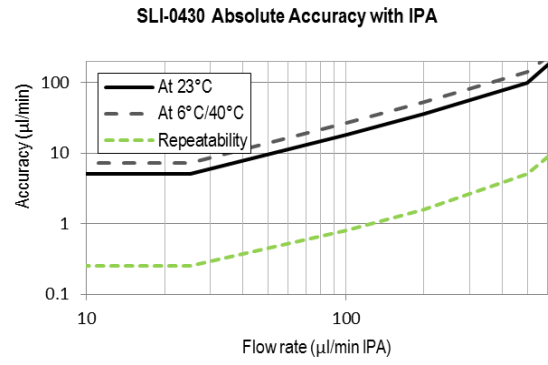
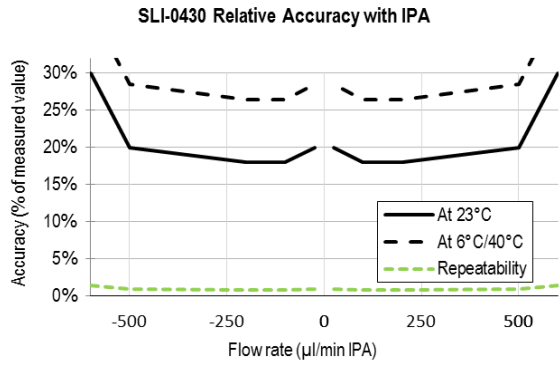


Figure 2: Flow meter accuracy and repeatability across the flow range. Relative error in % of measured value (left column) and absolute error in  $\mu\text{l}/\text{min}$  or  $\text{ml}/\text{min}$  in case of the SLI-2000 (right column) for IPA